




WATER TESTING SOLUTIONS

Contour Comparator Tests

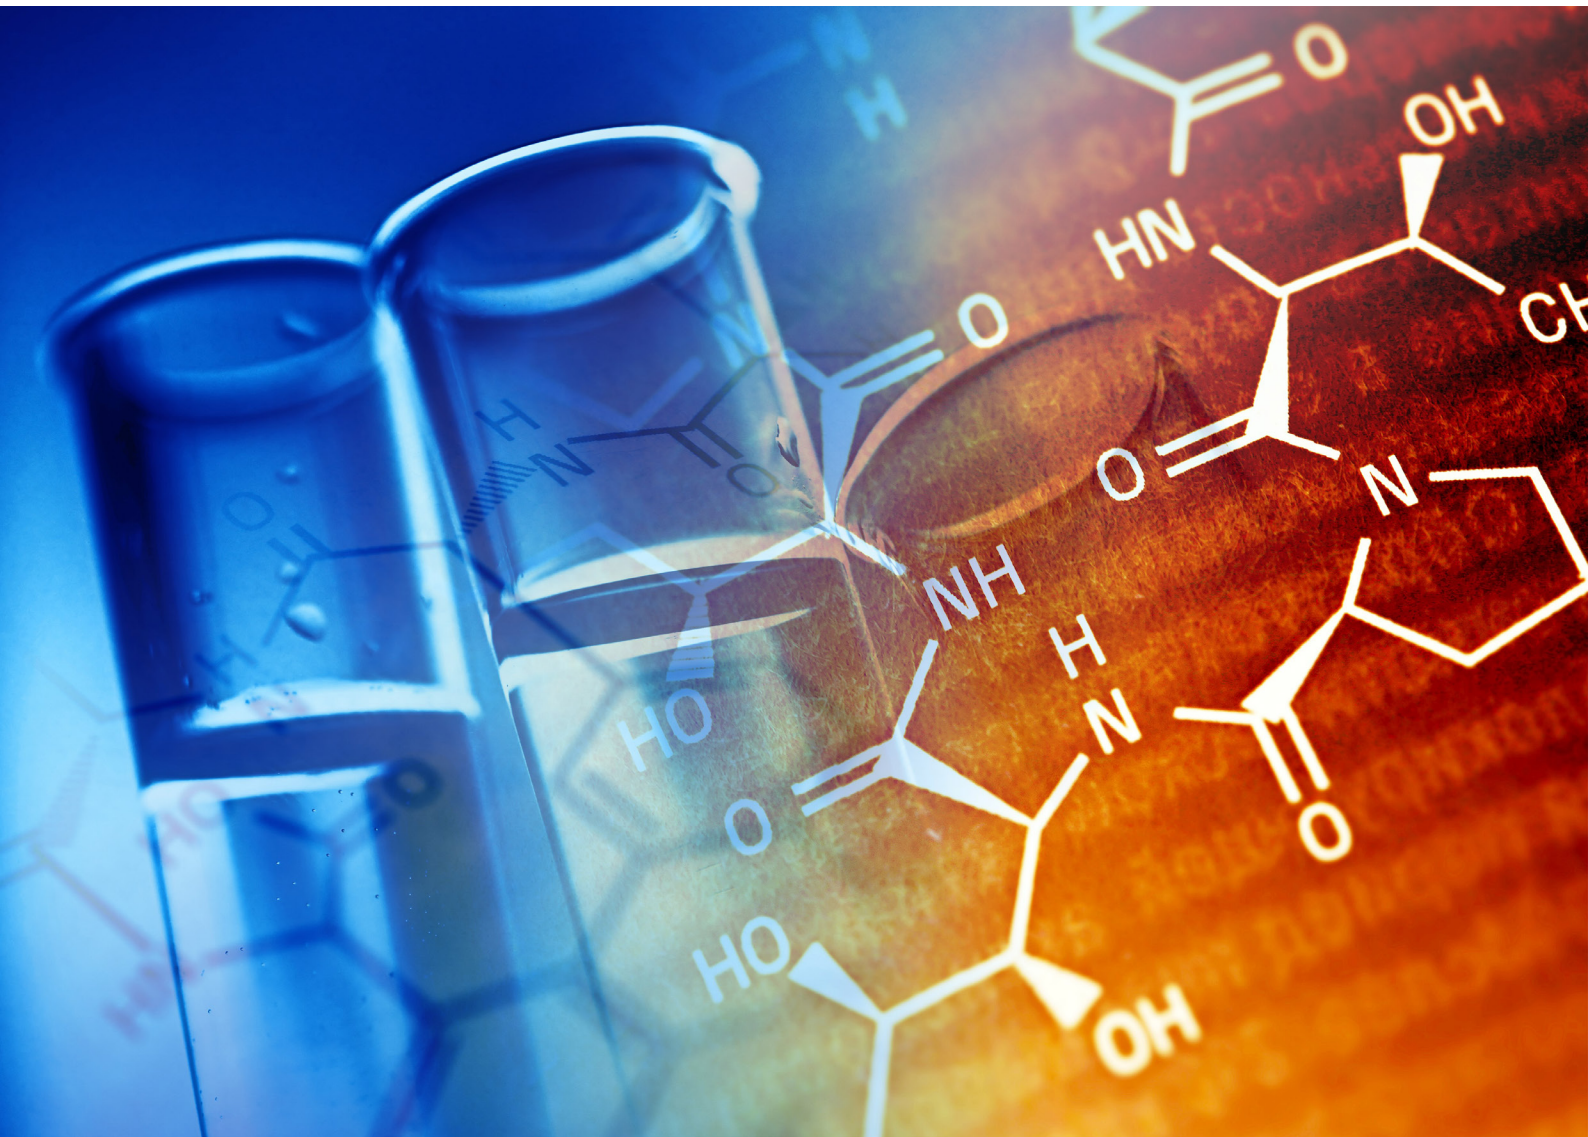

Water Testing Solutions Ltd

Unit 11, Wickham Business Centre, Harwood Road, Littlehampton, BN17 7AU. United Kingdom.

Tel: +44 (0)1903 714199 www.watertestingsolutions.com

Compact and versatile, the contour comparator offers simple visual testing with a wide range of test options. The contour comparator lines up the sample colour with the colour discs for an easy comparison, suitable for all users. The contour comparator kit utilises the globally recognised DPD method to provide clear colour development. The contour comparator has more than 40-disc options. Choose your disc options based on the tests you require.

Description	Range	Test Kit Code	Disc Code	Reagent Pack Code
Alkalinity (Alkavis)	0-250 mg/l CaCO ₃	WTS-K101935	WTS-B101995	WTS-P101965
Aluminium	0-0.5 mg/l Al	WTS-K101936	WTS-B101996	WTS-P101966
Ammonia	0-1 mg/l N	WTS-K101937	WTS-B101997	WTS-P101967
Bromine	0-8 mg/l Br ₂	WTS-K101938	WTS-B101998	WTS-P101968
Chlorine (free & total)	0-5 mg/l Cl ₂	WTS-K101939	WTS-B101999	WTS-P101969
Chlorine (free & total)	0-2 mg/l Cl ₂	WTS-K101940	WTS-B102000	WTS-P101970
Chlorine (free & total)	0-1 mg/l Cl ₂	WTS-K101941	WTS-B102001	WTS-P101971
Chlorine HR	0-50 mg/l Cl ₂	WTS-K101942	WTS-B102002	WTS-P101972
Chlorine HR	0-250 mg/l Cl ₂	WTS-K101943	WTS-B102003	WTS-P101973
Copper (Coppercol)	0-5 mg/l Cl ₂	WTS-K101944	WTS-B102004	WTS-P101974
Fluoride	0-1.5 mg/l F	WTS-K101945	WTS-B102005	WTS-P101975
Hydrogen Peroxide LR	0-1 mg/l H ₂ O ₂	WTS-K101946	WTS-B102006	WTS-P101976
Hydrogen Peroxide HR	0-100 mg/l H ₂ O ₂	WTS-K101947	WTS-B102007	WTS-P101977
Iron MR	0-10 mg/l Fe	WTS-K101948	WTS-B102008	WTS-P101978
Manganese	0-0.03 mg/l Mn	WTS-K101949	WTS-B102009	WTS-P101979
Manganese HR	0-5 mg/l Mn	WTS-K101950	WTS-B102010	WTS-P101980
Molybdate HR	0-100 mg/l MoO ₄	WTS-K101951	WTS-B102011	WTS-P101981
Nitrate (Nitratetest)	0-15 mg/l N	WTS-K101952	WTS-B102012	WTS-P101982
Nitrite (Nitricol)	0-0.4 mg/l N	WTS-K101953	WTS-B102013	WTS-P101983
Ozone	0-1.0 mg/l O ₃	WTS-K101954	WTS-B102014	WTS-P101984
Phosphate LR	0-4 mg/l PO ₄	WTS-K101955	WTS-B102015	WTS-P101985
Phosphate HR	0-100 mg/l PO ₄	WTS-K101956	WTS-B102016	WTS-P101986
Silica	0-4 mg/l SiO ₂	WTS-K101957	WTS-B102017	WTS-P101987
Sulphide	0-0.5 mg/l S	WTS-K101958	WTS-B102018	WTS-P101988
Zinc	0-4 mg/l Zn	WTS-K101959	WTS-B102019	WTS-P101989

Description	Range	Test Kit Code	Disc Code	Reagent Pack Code
pH Bromocresol Purple	pH 5.2-6.8	WTS-K101960	WTS-B102020	WTS-P101990
pH Bromothymol Blue	pH 6.0-7.6	WTS-K101961	WTS-B102021	WTS-P101991
pH Phenol Red	pH 6.8-8.4	WTS-K101962	WTS-B102022	WTS-P101992
pH Thymol Blue	pH 8.0-9.6	WTS-K101963	WTS-B102023	WTS-P101993
Universal pH	pH 4-11	WTS-K101964	WTS-B102024	WTS-P101994